


# SEATING TISSUE LOAD MANAGEMENT ALGORITHM



Note: This algorithm is meant as a guide, and is not a substitute for clinical judgment. Regardless of product selection, a full assessment of skin status and repositioning is required according to best clinical practice.

Seat/Back Combination Products for Prevention with Positioning  
LOW to MODERATE risk

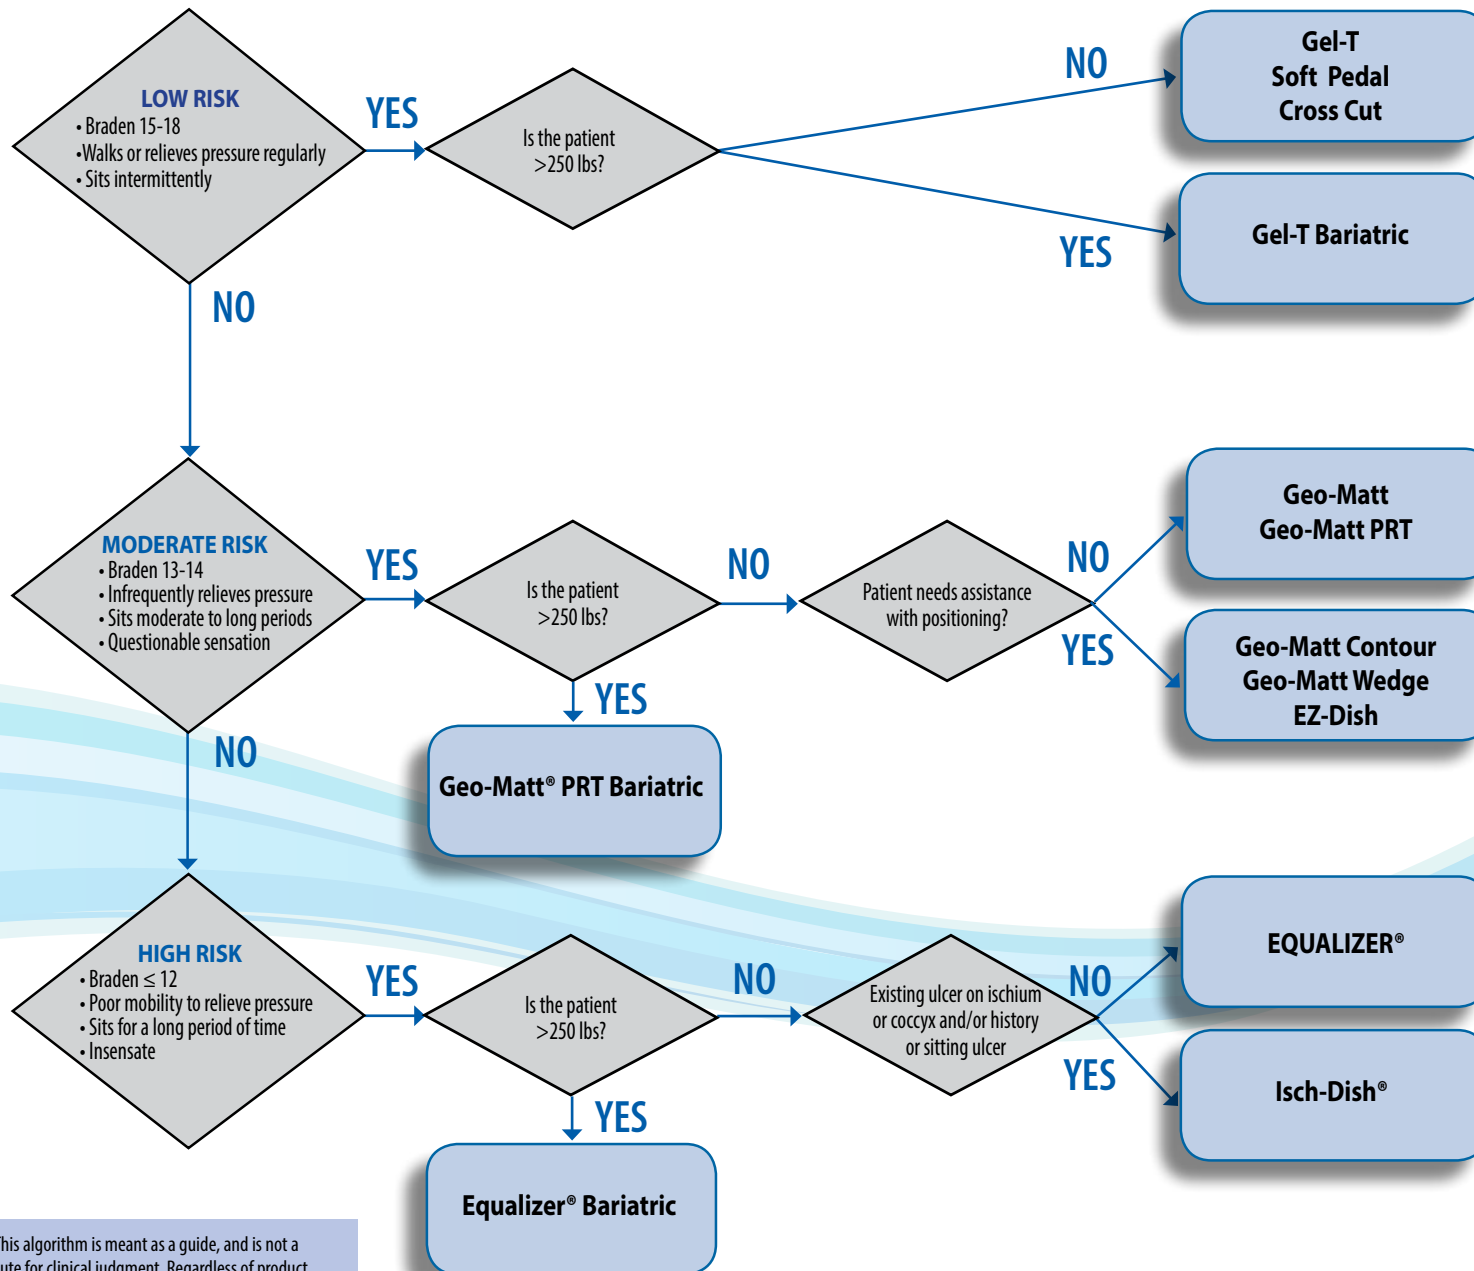

**Short Wave®**  
Seat and Back Cushion

**Geo-Wave®**  
Specialty Chair Cushion